Government Medicai Conege & Hospitai, Gondia कुवर तिलकसिंह सामान्य कम्णालय परिसर, नेहरू बाँक, गाँदिया, महाराष्ट्र-४४१६०१ Telephone No 07182 238090 Website: www.gmcgondia.in Email-ID:- gmcgstore-2094@gmail.com Ref. No./GMCSHG/HospitalPS/QV 5232 13030 Uate: 12 / 0 9 /2020 Open Quotation Notice Dean Govt. Medical College & Hospital, Gondia invites open quotation for the supply of Following Items from Manufacturer/Dealers, interested suppliers/Manufacturer/dealer can send their

quotation Quotation should be sent in sealed envelope (duly sealed by selling wax) by post or hand

delivery so as to reach this office on or before 21 00 20p to 13:00 pm Date 8 timing of the opening of quotation 25 08 20 at 13:30 pm at college council Hall. Representative of the supplier may attend the meeting by submitting authorization letter.

1. The word "Quotation" for Per Item Name and last Date / /2020 Should be clearly written on cover.

- 2. Quotation, which received late, will not be accepted under any circumstances.
- 3 Rate should be for free delivery at Govt. Medical College, Gondia premises only. Rate should be gupted including all charges. Rates must be quote on letter head along with Pan, VAT and CST Number.
- 4. Quoted goods should be strictly accordingly to the specification mentioned in the list. Make Model of items should be specifically stated in quotation and catalogue /leaflets etc. should be submit along with the quotation.
- 5 Catalogue/Leaflet is must quotation received and the price of the same will not be considered on leaflets/Catalogue
- 6. The concern Head of the Department can ask for demo of the lowest price model and it will be binding for the supplier to give the demo in stipulated period (i.e. within 4 days) at Gondia or nearby place. If the supplier fails to give the demonstration of the same model in stipulated period then his quotation will be treated as cancelled.
- 7. After placing the order to lowest one, the order will have to execute in full within the stipulated time if the supplier fail to comply, within stipulated period after giving the order may be cancelled and he will be declared defaulter and his any offer will not be consider in future.
- 8. The undersigned reserved the rights to accept or reject any or all quotation without giving any reason
- 9. The quotation should be sent in the name of the Dean, Govt. Medical College, Gondia.
- 10. For the CMP purpose (unregistered) supplier should submit copy of Pan Card, Cancelled Check.
- One photograph, & Bank Details.

	नाव	संख्या	कंपणी	किमंत
,	Covindien Corvac Tubes (Yellow Tops)	05		

सोवत स्पेशिफिकेशन जोडलेले आहे.

GOVERNMENT MEDICAL COLLEGE & HOSPITAL, GONDIA

10:01 - 10:01

25.前55.00.71%高

Serum-separating tubes, also known as serum separator tubes or SSTs, are used in medical clinical chemistry tests requiring blood serum.


SSTs are sometimes called 'marble-top tubes", "tiger-tops", or "gold-topped tubes", referring to the stoppers which are either gold, red with a gold ring on top, or marbled red and grey. Marble-top tubes are also referred to as "tiger-tops" in some clinics. SPS tubes have a paler colour, sometimes leading confusion; these are known as "yellow tops" not "gold". Trademarked versions Include Covidien "Corvaç" tubes.

They contain a special gel that separates blood cells from serum, as well as particles to cause blood to clot quickly. The blood sample can then be centrifuged, allowing the clear serum to be removed for testing.[1][2] These tubes should be used with care when

measuring drug or hormone levels because the drug or hormone may diffuse from the serum into the gel, causing a reduction in 111

6/8/2em

06/08/2020

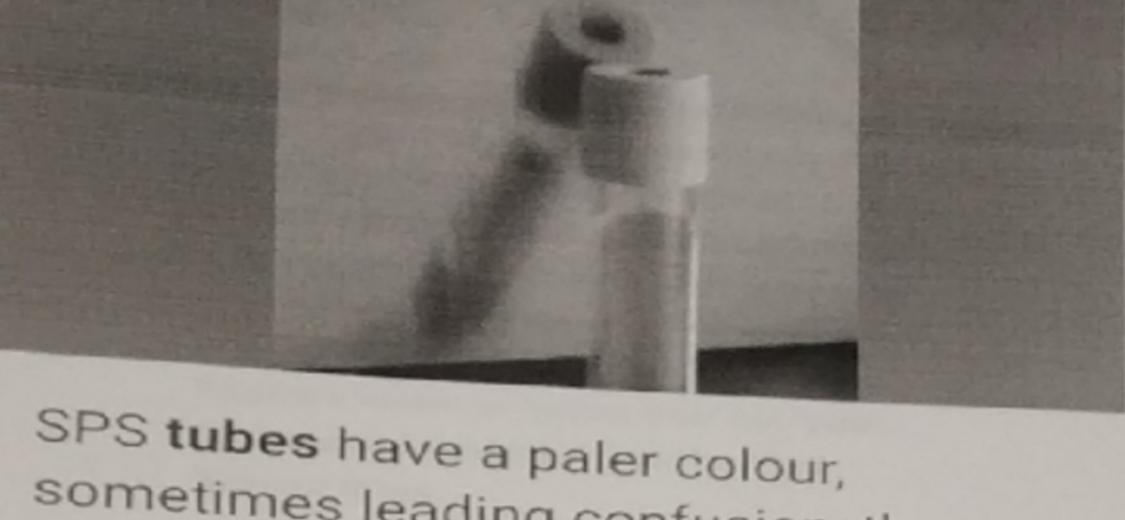

sometimes leading confusion; these are known as "yellow tops" not "gold". Trademarked versions include Covidien "Corvac" tubes. They contain a special gel that separates blood cells from serum, as well as particles to cause blood to clot quickly.